

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Serial No.: ARTL-0014
Location: SOUTH BRUNSWICK POLICE
Calibration File No.: 00443 Calib. Date: 02/17/2016 Calib. No.: 00033
Certification File No.: 00434 Cert. Date: 08/20/2015 Cert. No.: 00023
Linearity File No.: 00435 Lin. Date: 08/20/2015 Lin. No.: 00023
Solution File No.: 00442 Soln. Date: 02/09/2016 Soln. No.: 00167
Sequential File No.: 00443 File Date: 02/17/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUH S3-0079
Control Solution %: 0.100% Expires: 08/17/2017
Solution Control Lot: 15H143 Bottle No.: 0623

Coordinator

Last Name: GONCALVES First Name: MICHELLE MI: L
Signature: Sgt Michelle Goncalves #6040 Badge No.: 6040
Date: 02/17/2016

*Black Key Temperature Probe Serial.....# DDHHP2-055 (MA)
*Digital NIST Temperature Measuring System Serial.....# 150649677 (MA)

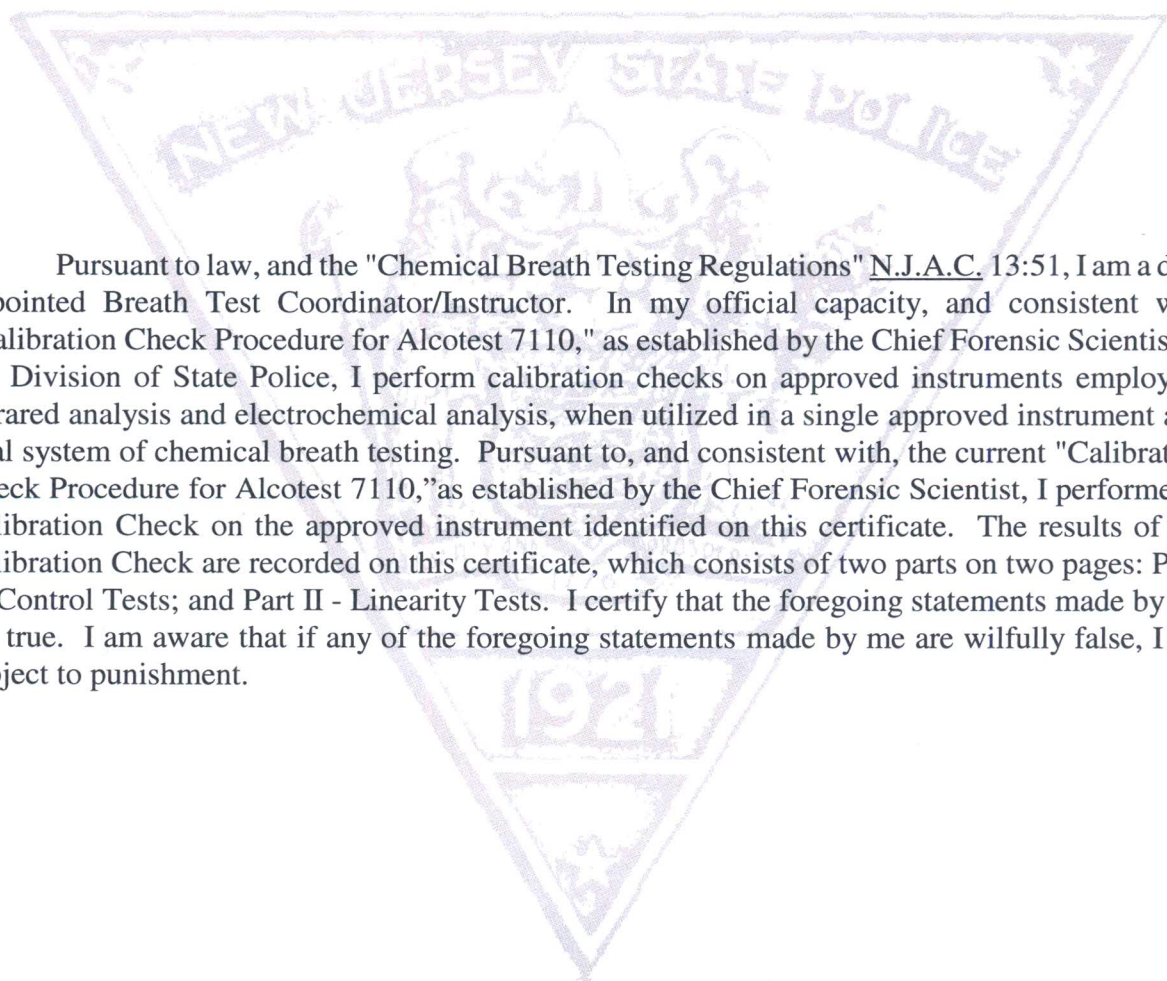

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

