


# Alcotest 7110 Calibration Record

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARTL-0014		
Location:	SOUTH BRUNSWICK POLICE				
Calibration File No.:	00433	Calib. Date:	08/20/2015	Calib. No.:	00032
Certification File No.:	00425	Cert. Date:	04/16/2015	Cert. No.:	00022
Linearity File No.:	00426	Lin. Date:	04/16/2015	Lin. No.:	00022
Solution File No.:	00432	Soln. Date:	08/10/2015	Soln. No.:	00160
Sequential File No.:	00433	File Date:	08/20/2015		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDUH S3-0079
Control Solution %:	0.100%			Expires:	09/23/2015
Solution Control Lot:	13I123			Bottle No.:	0811

## Coordinator

Last Name: GONCALVES      First Name: MICHELLE      MI: L  
Signature: Sgt. Michelle Goncalves #6040      Badge No.: 6040  
Date: 08/20/2015

\*Black Key Temperature Probe Serial.....# DDUNP2-231 (MA)  
\*Digital NIST Temperature Measuring System Serial.....# 130602271 (MA)

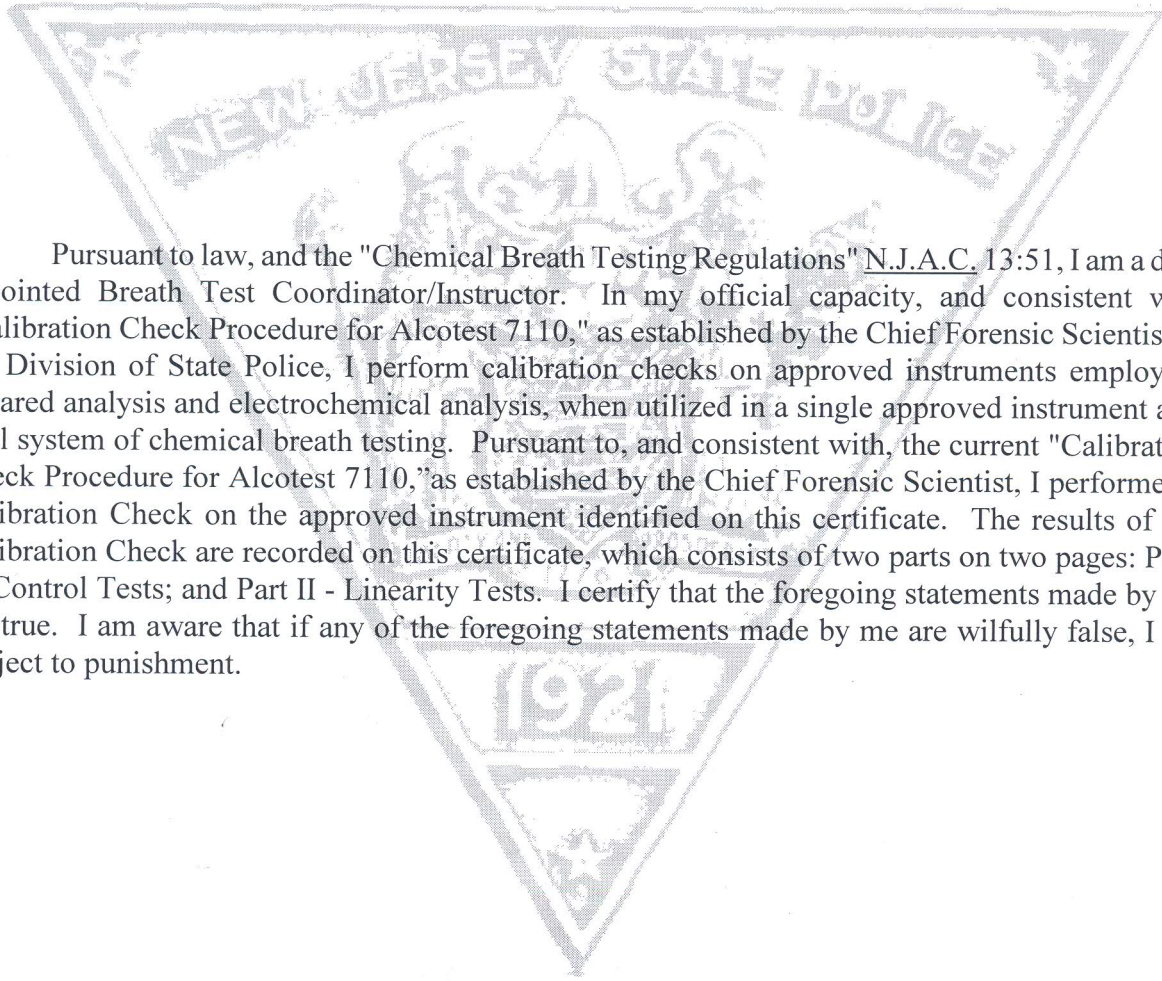

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

