

Alcotest 7110 Calibration Record

Equipment


Alcotest 7110 MKIII-C
Location: SOUTH BRUNSWICK POLICE
Serial No.: ARTL-0014
Calibration File No.: 00406
Calib. Date: 09/30/2014
Calib. No.: 00029
Certification File No.: 00395
Cert. Date: 05/01/2014
Cert. No.: 00020
Linearity File No.: 00396
Lin. Date: 05/01/2014
Lin. No.: 00020
Solution File No.: 00405
Soln. Date: 09/15/2014
Soln. No.: 00143
Sequential File No.: 00406
File Date: 09/30/2014

Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDUH S3-0079
Control Solution %: 0.100%
Expires: 09/17/2015
Solution Control Lot: 131122
Bottle No.: 0330

Coordinator

Last Name: GONCALVES
First Name: MICHELLE
MI: L
Signature: Sgt. Michelle Goncalves #6040
Badge No.: 6040
Date: 09/30/2014

*Black Key Temperature Probe Serial.....# DDXK P2-398 (new)
*Digital NIST Temperature Measuring System Serial.....# 130602271 (new)

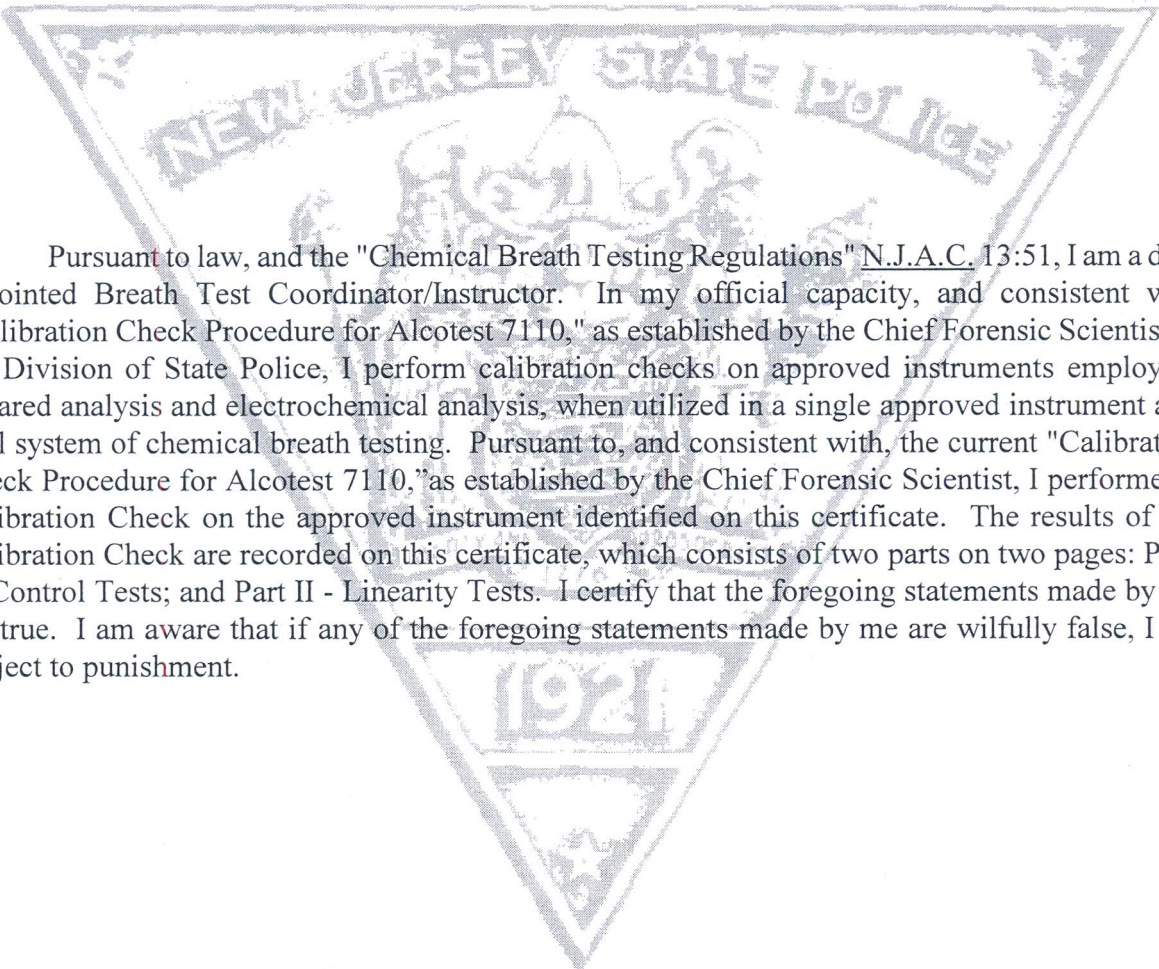

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

